


# Immunostaining in the OrganoPlate®


## 1. Objective

This protocol describes the immunostaining procedure of tissues grown in the OrganoPlate® 2-lane and 3-lane (see chip layout below)


OrganoPlate® 3-lane 40

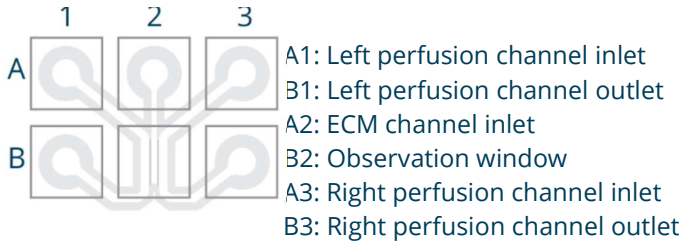

OrganoPlate® 3-lane 40

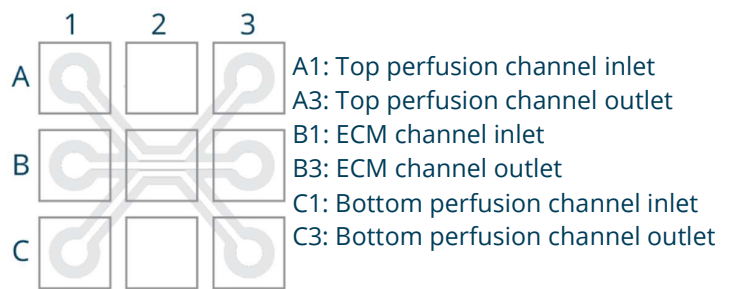

OrganoPlate® 2-lane 96



## 2. Background

Immunofluorescence staining is a technique that uses antibodies to target specific cellular biomolecules expressed on cells. Detection of the bound antibodies is done using fluorescence microscopy.

## 3. Materials

- Tween-20 (Sigma, cat# P9616)
- FBS (Gibco/ATCC, cat# A13450)
- Triton™ X-100 (Sigma, cat# T8787)
- HBSS (+Ca/Mg) (Sigma, cat# 55037C-1000ML)
- BSA (Sigma, cat# A2153)
- Crushed ice
- Repeating multichannel pipets and tips
- 1x PBS (Gibco, cat# 70013065)
- Rocker platform (optional)
- Fixative (see table 1)
  - Standard fixative is 3.7% formaldehyde (diluted 1:10 from stock, Sigma, cat# 252549-1L)

Fixative	Incubation time
3.7% formaldehyde in HBSS	10-15min RT
0.4% formaldehyde in HBSS	10-15min RT
-20°C 100% acetone	5min RT
-20°C 100% methanol	10-15min RT
-20°C 95% methanol, 5% acetic acid	5-10min RT

**Table 1.** Fixation methods compatible with the OrganoPlate®



- Permeabilization buffer: 0.3% Triton X-100 in PBS
- Blocking solution: 2% FBS, 2% BSA, 0.1% Tween20 in PBS
- Washing solution: 4% FBS in PBS
- Antibodies and nuclear stain (Hoechst™/DraQ5™)


## 4. Assay

### Fixation

Perform all steps at room temperature

1. Prepare fixative (see table 1)
  - a. Standard fixative is 3.7% formaldehyde in HBSS (dilute 1:10 from 37% stock)
  - b. Complete OrganoPlate® 2-lane: 21 mL
  - c. Complete OrganoPlate® 3-lane 40: 17 mL
  - d. Complete OrganoPlate® 3-lane 64: 25 mL
2. Aspirate medium from the chips and add fixative to the chips' inlets and outlets according to the volume scheme below.
  - OrganoPlate® 2-lane: 50  $\mu$ L to ECM inlet, 100  $\mu$ L to the perfusion channel inlet, 50  $\mu$ L to perfusion channel outlet
  - OrganoPlate® 3-lane 40 and 64: 100  $\mu$ L to tubule inlet, 50  $\mu$ L to all other inlets and outlets


**NOTE:** for tubular structures, it is important to have a difference in volumes from the inlet to the outlet to induce flow through the channel. The protocol details for tube on the top and right perfusion channel of the 3 lane-40 and 64 format as shown below (red for cell tubule, blue for ECM).

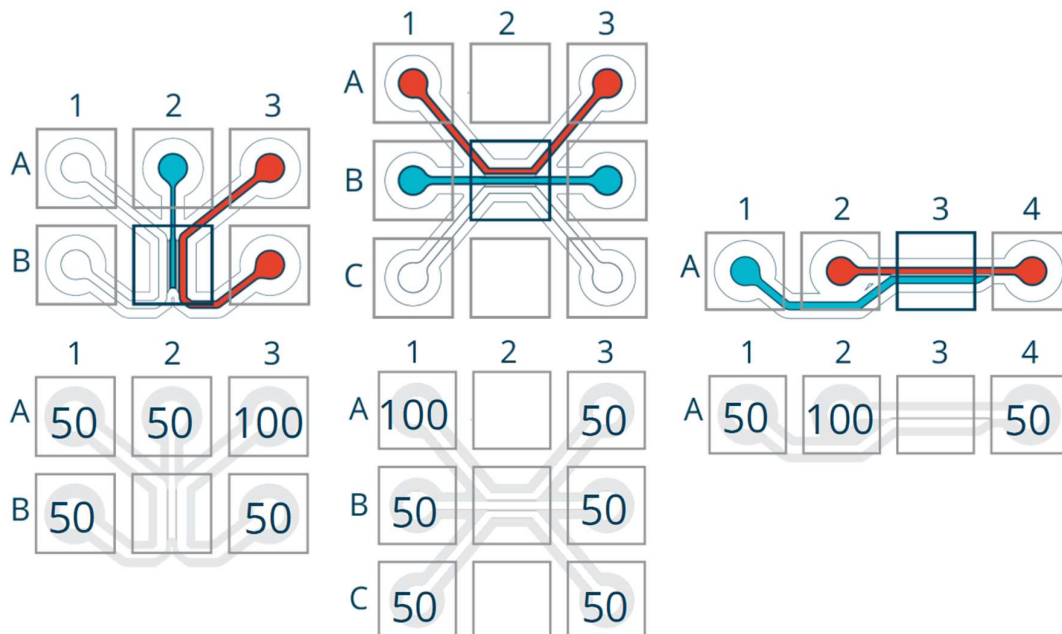


3. Incubate the fixative for the appropriate amount of time (see table 1)
4. Aspirate fixative and wash chips 2x (5 min each) with PBS using the volume scheme shown in step 2. Additionally, remove the HBSS from the observation window and replace with 1x PBS.



5. Proceed to immunostaining or seal the plate around the edges with Parafilm® and wrap the plate in aluminum foil. The fixed plate can be stored at RT up to 2 weeks. For optimal imaging quality, we recommend immediately proceeding with the antibody staining and image acquisition steps. Do not freeze the plate post fixation, as this will cause the glass bottom and the microfluidics to delaminate from the plate.
6. Prepare permeabilization buffer, blocking solution, and washing solution (see materials list)
7. Wash chips 1x 5 min with washing solution according to the volume scheme below.
  - a. OrganoPlate® 2-lane: 50  $\mu$ L to ECM inlet, 100  $\mu$ L to the perfusion channel inlet, 50  $\mu$ L to the perfusion channel outlet
  - b. OrganoPlate® 3-lane 40: 100  $\mu$ L to top perfusion channel inlet, 50  $\mu$ L to all other inlets and outlets
  - c. OrganoPlate® 3-lane 64: 100  $\mu$ L to right perfusion channel inlet, 50  $\mu$ L to all other inlets and outlets

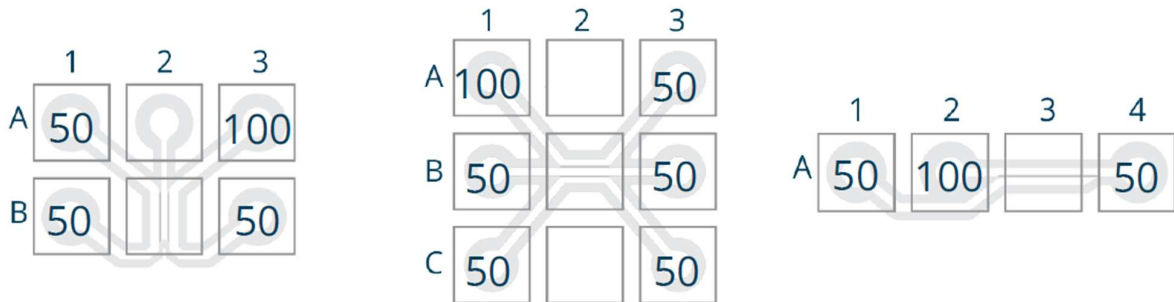

8. Aspirate the washing buffer and permeabilize cells for 10 minutes with permeabilization buffer according to the volume scheme shown in step 7
9. Aspirate permeabilization buffer and wash chips 1x 5 min with washing solution using the volume scheme shown in step 7
10. Aspirate washing buffer and block cells for 30-45 min with blocking solution according to the volume scheme shown in step 7
11. Meanwhile, prepare primary antibody in blocking solution in the appropriate dilutions
  - a. OrganoPlate® 2-lane: 40  $\mu$ L antibody per chip
  - b. OrganoPlate® 3-lane 40/64: 80  $\mu$ L antibody per chip
12. Aspirate blocking solution and add primary antibody solution according to the volume scheme below

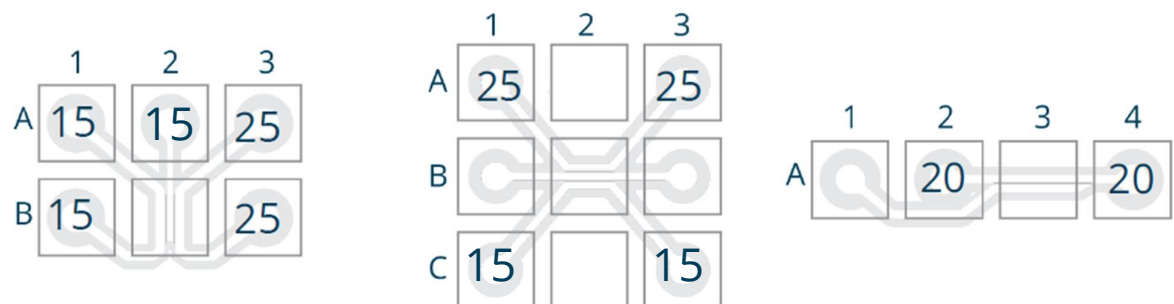


13. Incubate primary antibody on the rocker platform at RT (or at 4°C overnight if desired)
  - a. For tubular cultures, 1-2 hours of incubation on the rocker platform at RT is sufficient
  - b. For cultures of cells in gel, longer incubation times may be required (see troubleshooting section)


## Immunostaining

All steps are performed at room temperature unless specified otherwise.

To allow successful binding of primary and secondary antibodies, the antibody solution is perfused through the OrganoPlate® during antibody incubation steps. Perfusion can be created by placing the OrganoPlate® on a regular rocker platform and having it switch sides regularly. Use a small angle and a low switching interval (i.e. 5° angle, 2-5 min interval). Alternatively, flow can be induced by placing the OrganoPlate® under an angle by positioning one end on top of an object, e.g. a second 384 well plate (see figure on the right) and regularly switching sides manually.

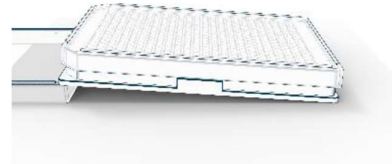

14. Meanwhile, prepare secondary antibody in blocking solution in the appropriate dilutions
  - a. OrganoPlate® 2-lane: 40 µL antibody per chip
  - b. OrganoPlate® 3-lane 40/64: 80 µL antibody per chip
15. Aspirate primary antibody solution and wash chips 2x (3 min each) with washing solution using the volume scheme shown in step 7
16. Aspirate washing solution and add secondary antibody solution according to the volume scheme shown in step 12
17. Incubate secondary antibody in the dark on the rocker platform at RT
  - a. For tubular cultures, 30 minutes of incubation on the rocker platform at RT is sufficient
  - b. For cultures of cells in gel, longer incubation times may be required (see troubleshooting section)
18. Aspirate secondary antibody solution and wash chips 2x (3 min each) with washing solution using the volume scheme described in step 7.
19. If desired, stain cells with direct stains (e.g. Hoechst or ActinRed), using manufacturer's instructions
  - a. Use stains for fixed cells
  - b. Use the volume scheme shown in step 12
  - c. Incubate stains on the rocker at RT at least 15 min for cells grown as tubes against the ECM gel and at least 30 min for cells embedded in ECM gel (see troubleshooting section)
20. Wash chips 1x (5 min) with PBS according to the volume scheme shown in step 7
21. Aspirate all wells and add 50 µL of PBS to all wells, following the scheme below

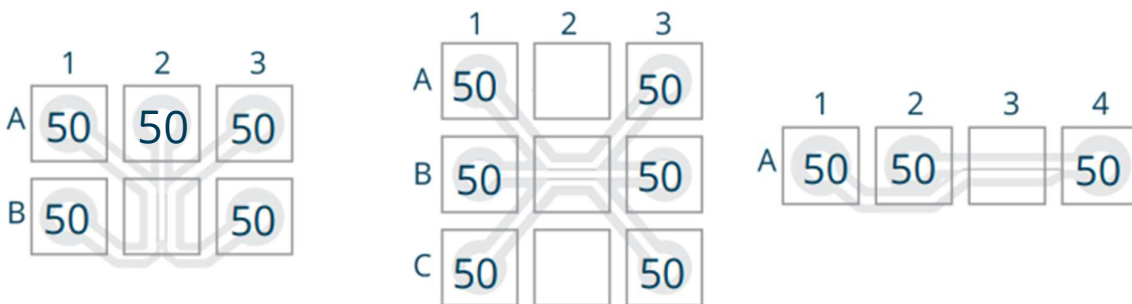

## 22. Proceed to microscopy

- a. Perform microscopy within one week after staining for optimal results, but preferably on the same day.
- b. Imaging can be performed on all standard fluorescent microscopes

### **Plate storage**

If the plate is not used immediately after fixation for antibody incubation or for imaging after the immunostaining is finished, the plate can be stored by sealing the edges with Parafilm and wrapping it with aluminium foil. Store the plate either at room temperature for up to two weeks or at 4°C for long term storage.

Never store the OrganoPlate® in the freezer or freeze existing cultures, as this will cause the glass bottom and the microfluidics to delaminate from the plate and liquid will leak out from the channels.

## **5. Troubleshooting**

### **Insufficient staining**


Depending on the setup of the culture, some cultures may require longer staining procedures to obtain optimal results, for example neuronal networks grown in Matrigel® in the OrganoPlate® 2- lane. For these types of cultures, the following measures can be taken to improve antibody staining:



- Addition of 1% Triton to the primary and secondary antibody solution (steps 11 & 14)
- Prolongation of incubation times
  - Incubate primary antibody for 2 days, on the rocker, at RT (step 13b)
  - Incubate secondary antibody for 2 days, on the rocker, at RT (step 17b)
  - Incubate nuclear stains for 1 day, on the rocker, at RT (step 19c)

**Note:** because these measures prolong the staining procedure significantly, use of aseptic technique is recommended to avoid growth of bacteria in the cultures. After fixation, work in a sterile cabinet and use sterile solutions (prepare solutions using only sterile components or filter buffers after preparation).



## Plate Layout

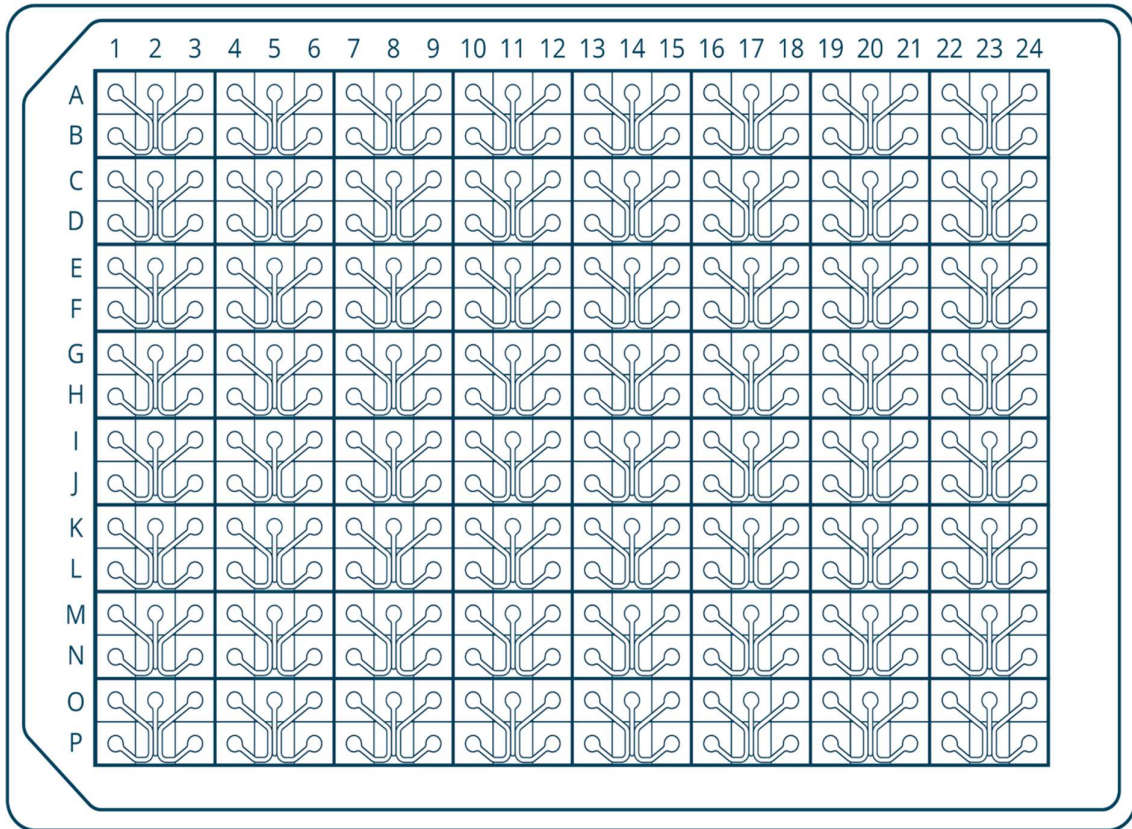

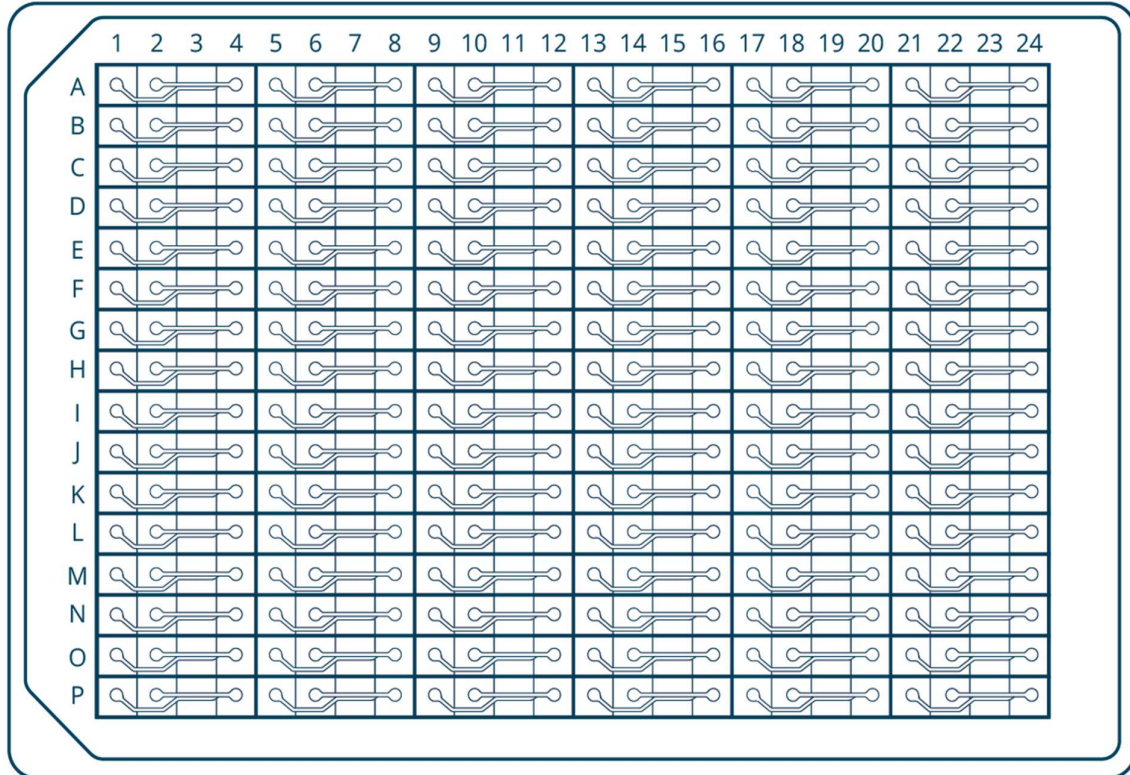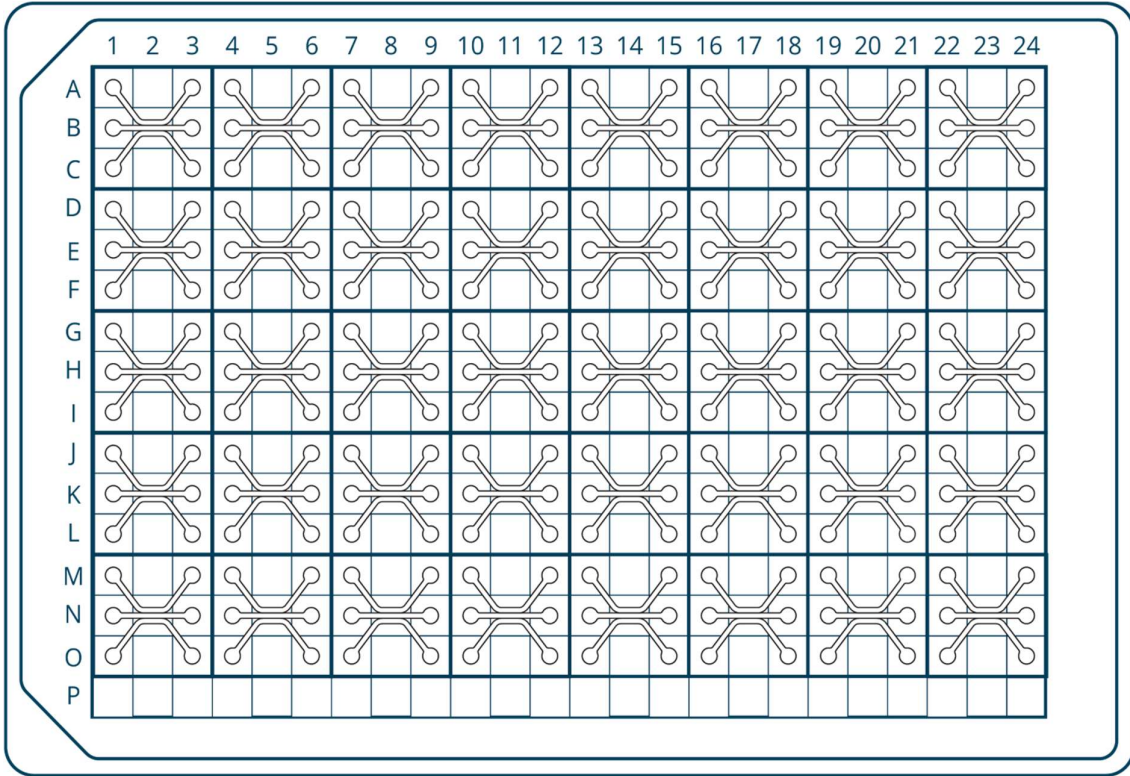

## MIMETAS Product List

<b>Cat. No.</b>	<b>Product Name</b>
MI-OR-CO-CU-01	OrganoReady® Collagen 3-lane 40
MI-OR-CO-CU-02	OrganoReady® Collagen 3-lane 64
MI-OR-CC-01	OrganoReady® Colon Caco-2 3-lane 40
MI-OR-CC-02	OrganoReady® Colon Caco-2 3-lane 64
MI-OR-BV-01	OrganoReady® Blood Vessel HUVEC 3-lane 40
MI-OR-BV-02	OrganoReady® Blood Vessel HUVEC 3-lane 64
MI-OR-AN-01	OrganoReady® Angiogenesis HUVEC 3-lane 64
MI-OR-HB-01	OrganoReady® BBB HBMEC 3-lane 40
MI-OR-HB-02	OrganoReady® BBB HBMEC 3-lane 64
MI-OR-VB-01	OrganoReady® Vascular Bed HUVEC
MI-OM-BVBM-01	OrganoMedium® HUVEC-BM
MI-OM-HBBM-01	OrganoMedium® HBMEC-BM
MI-OFPR-S	OrganoFlow® S
MI-OFPR-L	OrganoFlow® L
MI-OT-VP2	OrganoTEER® Standard package

### Contact information

**Purchasing:** [order@mimetas.com](mailto:order@mimetas.com)

**Customer service:** [info@mimetas.com](mailto:info@mimetas.com)

**Technical support:** [support@mimetas.com](mailto:support@mimetas.com)

This protocol is provided 'as is' and without any warranties, express or implied, including any warranty of merchantability or fitness for a particular purpose or assured results, or that the use of the protocol will not infringe any patent, copyright, trademark, or other proprietary rights. This protocol cannot be used for diagnostic purposes or be resold. The use of this protocol is subject to Mimetas' General Terms and Conditions of Delivery, Purchase and Use. For General Terms and Conditions, please visit <https://www.mimetas.com/en/company/terms-conditions/>

### MIMETAS Europe

De Limes 7  
2342 DH, Oegstgeest  
The Netherlands  
+31 (0)85 888 3161

### MIMETAS USA

704 Quince Orchard Road  
Suite 260, MD 20878,  
Gaithersburg, USA  
+1 (833) 646-3827

### MIMETAS Japan

4F Tekko Building, 1-8-2  
Marunouchi, Chiyoda-Ku  
Tokyo, 100-0005, Japan  
+81 3-6870-723

